



# SPECTROSCOPY LABORATORY




Glass samples fabricated by Sol-gel technique

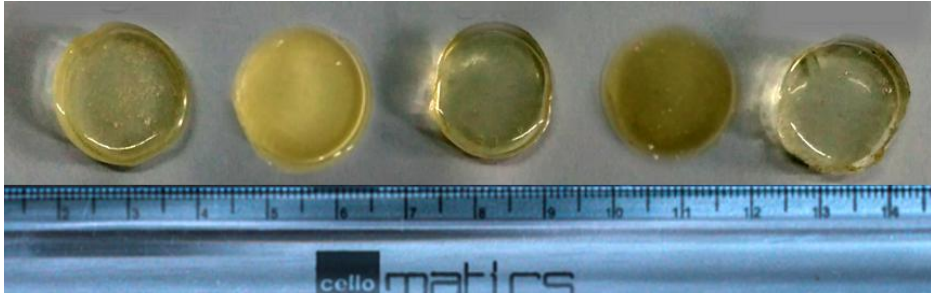


Fluoromax 4P Spectrofluorometer

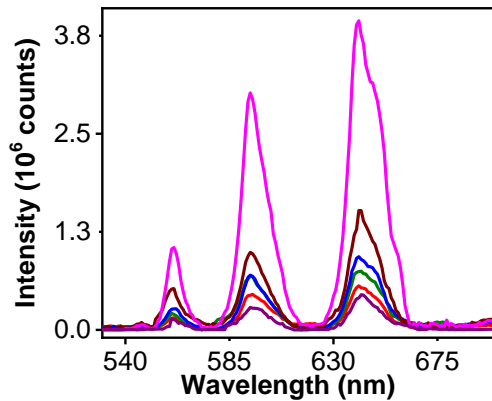

Photoluminescence spectra recorded for studied samples

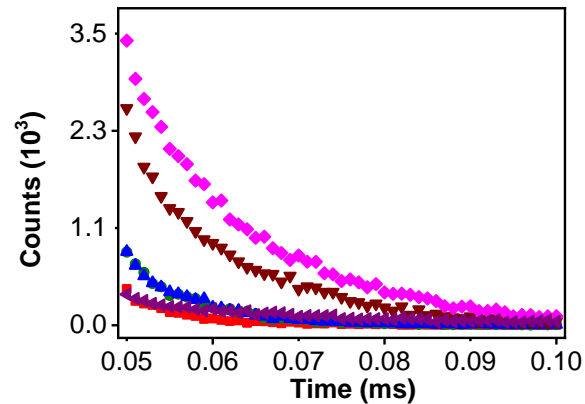

TCSPC recorded for studied samples

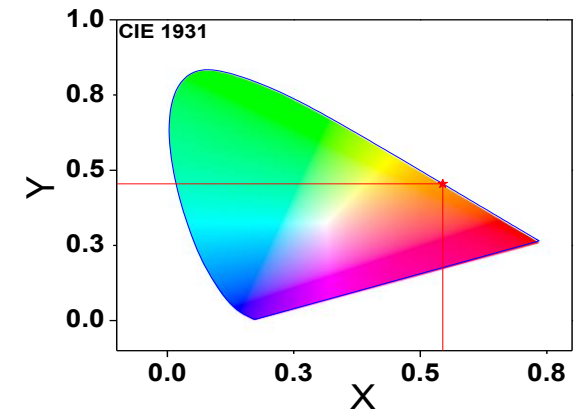

CIE chromaticity diagram recorded for a studied sample